



**CGS Analysen-
Mess- und
Regeltechnik
GmbH**

Keltenstraße 3
D-85095
Denkendorf
Telefon
08466/9415-0
Telefax
08466/9415-49

Documentation


**ANALYSER EQUIPMENT
ASU No. 9 Kosice
Mounting Plate QE74090**

**AIR LIQUIDE AGS GmbH
D-47805 Krefeld**

**Project-No.:
05/142
Order-No.:
4500025169**

revision list

[illegible]

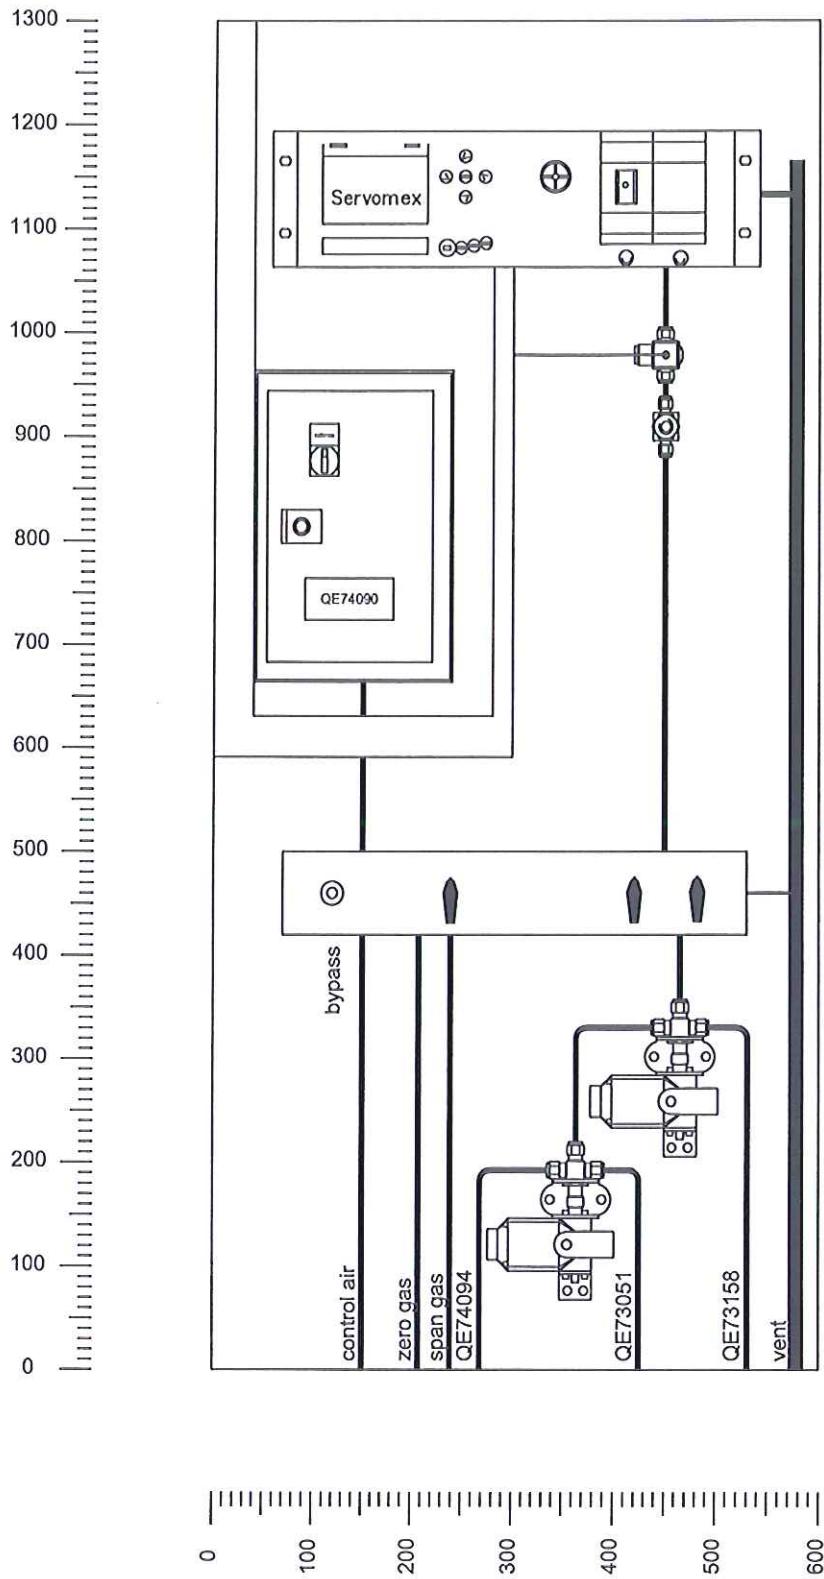


date		24.06.05	Drawn by		CGS GmbH	Air Liquide		mounting plate		ASU Kosice	project number		QE74090	
name		Wendlik	CGS GmbH		Keltenstr.3	Air Liquide ACS GmbH		QE74090		4500025169	drawing number		+	
drawing			CGS		D-85095 Denkendorf	Air Liquide ACS GmbH					sheet		03	
revision			time		05-142									
name														
name														

QE74090


Servomex 4100 C

range 1: 0-10 ppm O2
range 2: 0-1000 ppm O2

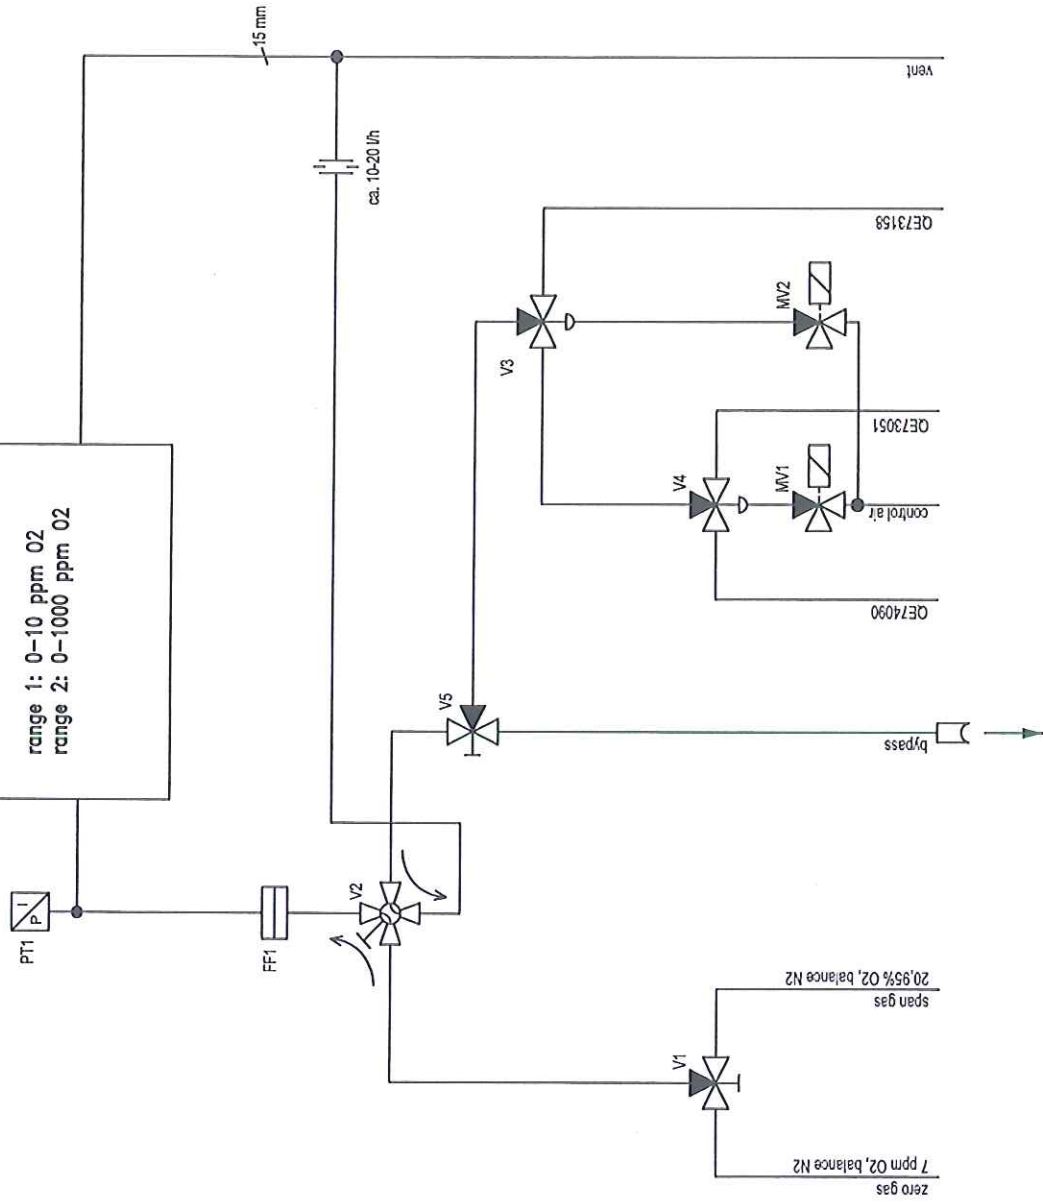


piping 6 mm stainless steel

[illegible]

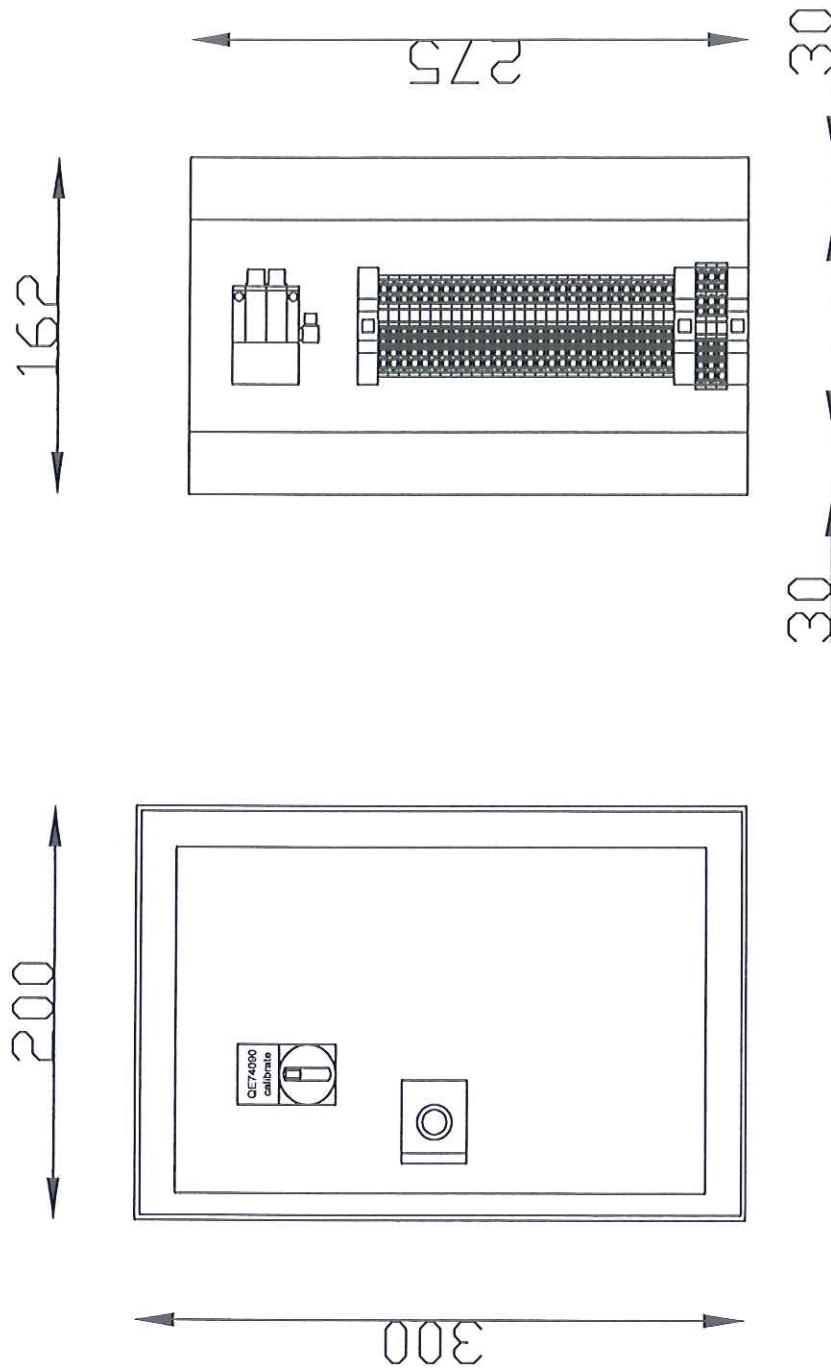[illegible]

[illegible]

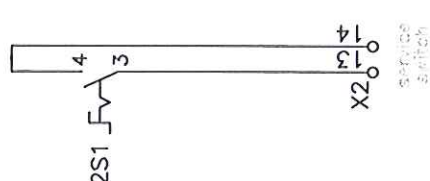[illegible]

